CERTIFICATE OF AN	ALYSIS	
Customer:	ACCURA' TEST LAB  Batch #: Laboratory Number:	Report Issue Date: Order Date: Analysis Date:
Sample Description: Unit Weight:	Photo	Extraction Technician: LL  Analytical Chemist: LL  Hernan Pristo  Laboratory Manager
CANNABINOID F  Analyte LOQ Results %	PROFILE  Analyte LOQ Result	S % Analyte LOQ Results %
Max Active	Canna	Active binoids
Max Active	Total Canna	lbinoids

Cannabidivarinic Acid(CBDVA) Cannabidivarin(CBDV) Cannabidiolic Acid(CBDA) Cannabigerolic Acid(CBGA) Cannabigerol(CBG) Cannabidiol(CBD)

Tetrahydrocannabivarin(THCV) Tetrahydrocannabivarinic Acid(THCVA) Cannabinol(CBN) Delta-9-Tetrahydrocannabinol(D9-THC) Delta-8-Tetrahydrocannabinol(D8-THC)

9S-Delta-10-Tetrahydrocannabinol(9S-D10-THC) 9R-Delta-10-Tetrahydrocannabinol(9R-D10-THC) 9S-Hexahydrocannabinol(9S-HHC) PR-Hexahydrocannabinol(9R-HHC)

Cannabichromene(CBC) Cannabichromenic Acid(CBCA) Tetrahydrocannabinolic Acid(THCA) Delta-9-Tetrahydrocannabinol(D9-THCP) Delta-8-Tetrahydrocannabinol-O-Acetate (D8-THCO)

Reporting Limits will vary based on sample extraction weight used for the analysis. Accurate Test Lab, LLC utilizes based upon traceable Reference Standards and Certified Reference Material to calibrate analytical instruments along with proven analytical methods. The methods are applied in the most ethical manner following good laboratory practice guidelines.

The results of this report are based solely on the sample submitted and cannot be reproduced. Results only apply to samples within COA as received.

Certificate of Analysis shall not be reproduce except in full without approval of Accurate Test Lab, LLC.

N/D: Not Detected LOQ: Limit of quantification

Analysis Method: ATL-LCM-001. Accurate Test Lab estimated expanded uncertainty is 13% as per in VALIDATION AND VERIFICATION OF ATL-LCM-001 (ATL-500A)





**CERTIFICATE OF ANALYSIS Report Issue Date:** Batch #: **Order Date: Customer: Analysis Date: Laboratory Number:** Extraction Technician: HP Sample Description: Analytical Chemist: HP **Photo Unit Weight:** Hernan Pristo Laboratory Manager RESIDUAL SOLVENTS PROFILE Concentration **Action Limit** PASS/FAIL **Analyte** (PPM) (PPM)

**NOTES** 

Reporting Limits will vary based on sample extraction weight used for the analysis. Accurate Test Lab, LLC utilizes based upon traceable Reference Standards and Certified Reference Material to calibrate analytical instruments along with proven analytical methods. The methods are applied in the most ethical manner following good laboratory practice guidelines.

The results of this report are based solely on the sample submitted and cannot be reproduced. Results only apply to samples within COA as received.

Certificate of Analysis shall not be reproduce except in full without approval of Accurate Test Lab, LLC.

N/D: Not Detected LOQ: Limit of quantification

Analysis Method: ATL-GCM-001

1-Pass/Fail statement is based on California Code of Regulations, Title 16, Section 5718. Accurate Test Lab estimated expanded uncertainty is 25%, Following NIST, EURACHEM & CITAC guidelines.



## **CERTIFICATE OF ANALYSIS ACCURATE Report Issue Date:**

Batch #: **Customer: Order Date: Analysis Date: Laboratory Number:** 

Extraction Technician: HP Sample Description: Analytical Chemist: HP

**Photo** 

**Unit Weight:** Hernan Pristo

## **PESTICIDES PROFILE**

**Analyte** RESULT PASS/FAIL **Analyte** RESULT PASS/FAIL **Analyte** RESULT PASS/FAIL




**NOTES** 

Reporting Limits will vary based on sample extraction weight used for the analysis. Accurate Test Lab, LLC utilizes based upon traceable Reference Standards and Certified Reference Material to calibrate analytical instruments along with proven analytical methods. The methods are applied in the most ethical manner following good laboratory practice guidelines. The results of this report are based solely on the sample submitted and cannot be reproduced. Results only apply to samples within COA as received. Certificate of Analysis shall not be reproduce except in full without approval of Accurate Test Lab, LLC. N/D: Not Detected T:Trace Cannabinoids detected but are below limit of quantification.



Laboratory Manager

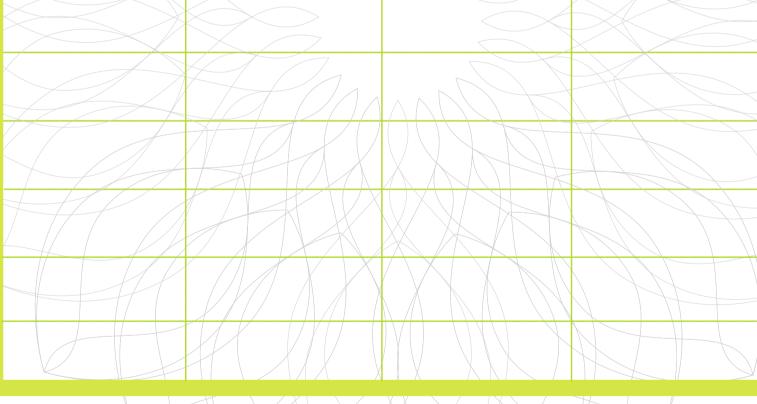


**NOTES** 

Reporting Limits will vary based on sample extraction weight used for the analysis. Accurate Test Lab, LLC utilizes based upon traceable Reference Standards and Certified Reference Material to calibrate analytical instruments along with proven analytical methods. The methods are applied in the most ethical manner following good laboratory practice guidelines. The results of this report are based solely on the sample submitted and cannot be reproduced. Results only apply to samples within COA as received. Certificate of Analysis shall not be reproduce except in full without approval of Accurate Test Lab, LLC. ND:Not Detected - NA:Not Analyzed - CFU:Colony-forming unit / Analysis Method: ATL-PHI-001 / Accurate Test Lab estimated expanded uncertainty is less than 10%



CERTIFICATE OF ANALYSIS **Report Issue Date:** Batch #: **Order Date:** Customer: **Analysis Date: Laboratory Number:** Extraction Technician: HP Sample Description: Analytical Chemist: HP **Photo Unit Weight:** Hernan Prieto Laboratory Manager **MICROBIOLOGY ANALYSIS** Microbe(s) **CFU Detected** Limit of Detection (CFU/g) CFU/g PASS / FAIL

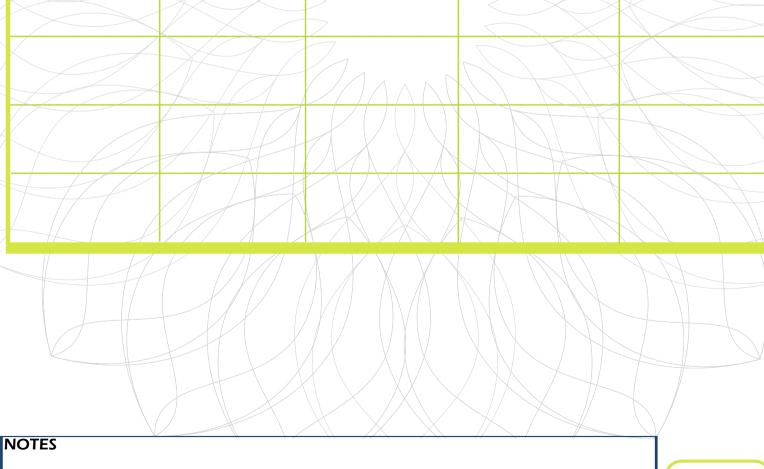

Reporting Limits will vary based on sample extraction weight used for the analysis. Accurate Test Lab, LLC utilizes based upon traceable Reference Standards and Certified Reference Material to calibrate analytical instruments along with proven analytical methods. The methods are applied in the most ethical manner following good laboratory practice guidelinesThe results of this report are based solely on the sample submitted and cannot be reproduced. Results only apply to samples within COA as received.

Certificate of Analysis shall not be reproduce except in full without approval of Accurate Test Lab, LLC.

TNTC: Too numerous to count - ND: Not Detected - NA: NotApplicable -GFU:Colony-forming unit 1-Pass/Fail criteria based on CMTL sample testing Florida Department of Health

Emergency Rule for 2020, Pass: Results within limits /specifications, Fail: Results exceed limits/specifications Accurate Test Lab estimated expanded uncertainty(CFU/g):-Aerobic Plate

Count: 10 -Staphylococcus Aureus: 4 - Yeast: 4 - Mold: 2 - Enterobacteriaceae: 6. Analysis Method: ATL-PHI-002

