

bebalance+ 1.6 560X12=V1.6

EN Instructions for use (qualified personnel)	3
---	---

INFORMATION

Date of last update: 2022-04-11

- ▶ Please read this document carefully before using the product and observe the safety notices.
- ▶ Please contact the manufacturer if you have questions about the product or in case of problems.
- ▶ Report each serious incident related to the product to the manufacturer and to the relevant authority in your country. This is particularly important when there is a decline in the health state.
- ▶ Please keep this document for your records.

The "560X12=V1.6 bebalance+ 1.6" adjustment software is referred to simply as bebalance+, software or adjustment software below.

Only put the product into use in accordance with the information contained in the accompanying documents supplied.

2 Product description

2.1 Function

The software is used to adjust the bebionic hand EQD, bebionic hand Short Wrist and bebionic hand Flex.

Various control programmes and switching methods are available for optimum adaptation to the patient.

Communication between the software and the prosthesis takes place exclusively via Bluetooth data transfer.

2.2 Combination possibilities

Supported Bluetooth adapter

- Bluetooth adapter "Bluetooth Long Range Dongle B33061"

Products that can be adjusted

- 8E70=*, 8E71=*, 8E72=*

3 Intended use

3.1 Indications for use

The software allows for patient-specific adaptation of the bebionic hand control device.

3.2 Conditions of use

The software is intended exclusively for adjusting the bebionic hand in the course of unilateral or bilateral fittings of the upper limbs.

The B33061 Bluetooth Long Range Dongle is the only permissible method of data transfer between the system components. It can be purchased from Ottobock.


An existing RF dongle can be used only for older bebionic hands of the M and L models.

3.3 Contraindications

- All conditions which contradict or go beyond the specifications listed in the section on "Safety" and "Indications for use".

4 Safety

4.1 Explanation of warning symbols

 **CAUTION** Warning regarding possible risks of accident or injury.

4.2 Structure of the safety instructions

 **CAUTION**

The heading describes the source and/or the type of hazard

The introduction describes the consequences in case of failure to observe the safety instructions. Consequences are presented as follows if more than one consequence is possible:

- > E.g.: Consequence 1 in case of failure to observe the hazard
- > E.g.: Consequence 2 in case of failure to observe the hazard
- ▶ This symbol identifies activities/actions that must be observed/carried out in order to avert the hazard.

4.3 General safety instructions

 **CAUTION**

Non-observance of safety instructions

Personal injury/damage to the product due to using the product in certain situations.

- ▶ Observe the safety instructions and the stated precautions in this accompanying document.

 **CAUTION**

Operator errors during the adjustment process

Injury due to unexpected prosthesis behaviour.

- ▶ Do not charge the prosthesis battery during the adjustment process since the prosthesis is not functional while the battery is being charged.
- ▶ The prosthesis must not remain unattended during the adjustment process while connected to the adjustment software and when being worn by the patient.
- ▶ Observe the maximum range of the Bluetooth connection and note that obstacles may limit this range.
- ▶ The Bluetooth dongle must not be unplugged from the computer during data transfer.
- ▶ Inform the patient immediately if the data connection is accidentally interrupted during the adjustment process.
- ▶ The connection to the prosthesis must always be disconnected after adjustments have been completed.
- ▶ Participation in an Ottobock product training course is recommended.
- ▶ Use the online help which is integrated into the software.

 **CAUTION**

Errors while establishing a connection with the prosthesis

Injury resulting from connection with more than one or the wrong prosthesis.

- ▶ When establishing a connection using the RF dongle, make sure only one RF device is activated in the immediate vicinity.

5 Scope of delivery

- 1 pc. "560X12=V1.6 bebalance+1.6" USB data carrier
- 1 pc. Instructions for use (qualified personnel)

6 System Requirements

6.1 Minimum PC Hardware Requirements

The minimum hardware requirements for installation/use of the adjustment software apply independently of the operating system being used. If the minimum requirements for using the operating system are higher than the hardware requirements described here, the minimum requirements for the operating system apply.

For 64-bit platforms

- PC with an Intel Core2 processor (x64) or faster
- 2 GB RAM
- At least 5 GB free hard drive space
- Graphics card with Open GL support
- Resolution 1280 x 768
- Display scale 100% or 96 DPI
- 32-bit colour depth (16.7 million colours)
- 1 free USB connection 2.0 or higher
- Mouse and keyboard

6.2 Supported operating systems

The following 64-bit operating systems are supported:

INFORMATION

32-bit operating systems are no longer supported.

- Microsoft Windows 10
- Microsoft Windows 11

INFORMATION

Please note that the latest bebalance+ USB driver version must always be installed for establishing the Bluetooth connection. You can download the latest driver version from the following site: www.ottobock.com.

6.3 Additional Installed Software Components

The following additional software components are required and installed during installation of the software (if they are not already installed on the PC):

- Microsoft .NET Framework 4.0

INFORMATION


Before the installation is started, the installation program checks if there is sufficient free space on the hard drive and returns an error message if this is not the case. If this occurs, a corresponding amount of space must be freed up on the hard drive. All components required by the Ottobock software are copied to the hard drive automatically by the installation program.

7 Installation

Installation information

- Please note that observing the prescribed system requirements is mandatory.
- It is recommended that you do not run any other programs during installation and use of the adjustment software, since this can affect performance.
- You must have administrator rights to install the software.


Carrying out the installation

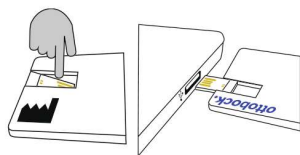

- 1) Start Microsoft Windows.
- 2) If necessary, poke the USB data carrier out from the card.
INFORMATION: The data carrier cannot be detached from the card.
- 3) Connect the data carrier to a freely accessible USB connection. The golden contacts should face upwards.
→ Microsoft Windows will automatically recognise the data carrier.
- 4) Follow the on-screen instructions to perform the installation.

INFORMATION

The installation does not start automatically

- ▶ Open "Computer" (key combination [Windows logo key]+E)
- ▶ Click the folder with the Data Station symbol .
- ▶ Start the installation by double-clicking "setup" or "setup.exe".

After the installation program starts, follow the on-screen instructions.

Information: fields marked with an asterisk (*) are mandatory.

INFORMATION

Cybersecurity

- ▶ Keep your operating system up to date and always install any available security updates.
- ▶ Protect your computer from unauthorised access (e.g., by using virus scans, password protection etc.).
- ▶ Do not use unsecured networks.
- ▶ Please contact the manufacturer if you suspect cybersecurity problems.

8 Data Transfer between the Prosthesis and PC

⚠ CAUTION

Errors while establishing a connection with the prosthesis

Injury resulting from connection with more than one or the wrong prosthesis.

- ▶ When establishing a connection using the RF dongle, make sure only one RF device is activated in the immediate vicinity.

Product settings using the adjustment software can only be made via Bluetooth data transfer. In order to do so, a Bluetooth wireless connection must be established between the product and the PC.

INFORMATION

Do not disconnect the Bluetooth dongle from the PC when there is an active Bluetooth connection.

8.1 Establishing a Bluetooth Connection to the Prosthesis


Carry out the following steps to activate the Bluetooth function of the prosthesis:


- > The prosthesis is switched on.
- ▶ Press and hold the program switch of the prosthesis for at least six seconds.
- Two beeps/vibration signals indicate that the Bluetooth function of the prosthesis has been activated successfully.


9 Starting the Program

INFORMATION

To run the software, ensure that the user is logged on to the PC with at least standard user rights.

- Double-click the  icon on the desktop.
- The program starts.

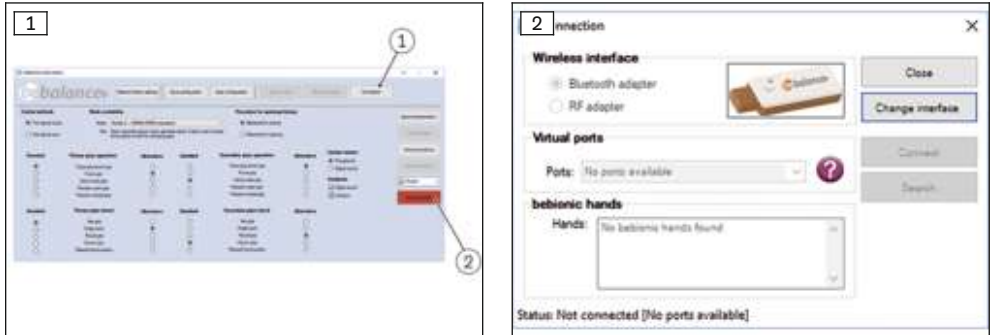

- 1) Click the "Connection" button (see fig. 1, item 1) in the main menu.
 - Another window appears (see fig. 2).
- 2) Select the appropriate adapter under "Wireless interface".
INFORMATION: Ottobock bebionic: Use the Bluetooth adapter (B33061 Bluetooth Long Range Dongle).
INFORMATION: Steeper bebionic: Use the Bluetooth adapter (B33061 Bluetooth Long Range Dongle) for the size "Small". Use the RF dongle for the size "Medium/Large".
- 3) Depending on the adapter used, click the "Use Bluetooth" or "Use RF adapter" button.
 - The sub-items "Ports" and "bebionic components" are added to the window.
 - When the RF adapter is used, the component is searched automatically and displayed in the list.
- 4) Click the "Search" button.
 - This starts a search for bebionic components.
- 5) The bebionic hand to be used appears in the "bebionic components" sub-item.
- 6) Select the hand to be used in the list.
- 7) Click the "Connect" button.
 - The main menu displays  (see fig. 1, item 2).

10 Closing the Program

The following options are available for closing the program:

- Click the "X" button in the top right corner of the program window
- Press the key combination [Alt+F4]

11 Uninstalling

To uninstall the Ottobock software, use the Windows uninstall function.

12 Further Information

12.1 Information Regarding the Online Help

The online help can be accessed via the **F1** button or the homepage.

12.2 Obtaining Program Version Information

The current program version of the installed software can be obtained from the homepage. You should have this information available whenever you contact software support.

12.3 Software Updates

Software and driver updates will be made available for free at regular intervals.

- 1) Make sure you are connected to the internet and go to the "<http://ottobock.com/en/datastation/>" website.
→ The webpage for the "Data Station" software will open.
- 2) Search for the description of the software that is to be updated under "Application/Patch".
- 3) Search for the applicable version.
- 4) Click "Download" in the column on the right in order to download the update.
- 5) Extract the "ZIP file" and execute it.

13 Trademarks

All product names mentioned in this document are subject without restriction to the respective applicable trademark laws and are the property of the respective owners.

All brands, trade names or company names may be registered trademarks and are the property of the respective owners.

Should trademarks used in this document fail to be explicitly identified as such, this does not justify the conclusion that the denotation in question is free of third-party rights.

Microsoft, Outlook and Windows are registered trademarks of Microsoft Corporation.

Pentium, Intel and Intel Core are registered trademarks of Intel Corporation.

14 CE conformity

Otto Bock Healthcare Products GmbH hereby declares that the product is in compliance with applicable European requirements for medical devices.

The full text of the regulations and requirements is available at the following Internet address:
<http://www.ottobock.com/conformity>

15 Symbols Used



Manufacturer



Article number



Declaration of conformity according to the applicable European directives



UDI number (Unique Device Identifier)

Licence Agreement

Manufacturer: Otto Bock Healthcare Products GmbH, Brehmstraße 16, 1110 Vienna, Austria.

PLEASE READ THIS END USER LICENCE AGREEMENT ("TERMS OF USE" OR "LICENCE AGREEMENT") CAREFULLY BEFORE YOU INSTALL OR USE THE OTTOBOCK SOFTWARE. BY INSTALLING OR USING THE OTTOBOCK SOFTWARE, YOU ARE AGREEING TO THE TERMS AND CONDITIONS OF THIS TERMS OF USE.

DO NOT USE THE OTTOBOCK SOFTWARE UNLESS YOU AGREE TO THE TERMS AND CONDITIONS OF THIS LICENCE AGREEMENT. IF YOU DO NOT AGREE TO THE TERMS AND CONDITIONS OF THIS LICENCE AGREEMENT, YOU CAN RETURN THE OTTOBOCK SOFTWARE TO THE LOCATION WHERE YOU ACQUIRED

THE SOFTWARE. IF YOU ACQUIRED THE OTTOBOCK SOFTWARE JOINTLY AND IN CONJUNCTION WITH HARDWARE, YOU CAN RETURN BOTH THE HARDWARE AND THE SOFTWARE.

IF YOU DO NOT AGREE TO THE TERMS AND CONDITIONS OF THESE TERMS OF USE, YOU ARE NOT AUTHORISED TO INSTALL OR USE THE OTTOBOCK SOFTWARE.

1. Contractual partners and object of the agreement

1.1 By accepting these Terms of Use, you are entering into a contract between yourself and the named Ottobock company (hereinafter also "Ottobock"); however, if you are acting on behalf of a company when installing or using the Ottobock software (e.g. as an employee of said company), the contract is concluded between the company and Ottobock (in which case "you" refers to said company). In case of any doubt, you are a party to the contract.

1.2 The licence covers the Ottobock software, including any related documentation (referred to as "Ottobock Software" below). The terms and conditions of this licence agreement also apply to any updates to the Ottobock software that replace or amend the original software – where Ottobock provides them to you after the installation of the Ottobock software – unless such an update is the object of a separate licence agreement. Any possible maintenance of the Ottobock software or other Ottobock products is not covered by this agreement; a separate agreement is required.

1.3 To the extent that the Ottobock software will be used to provide recommendations regarding patient fittings (e.g. for certain adjustments to Ottobock products after taking customer measurements), please note that such suggestions merely represent non-binding recommendations from Ottobock. While Ottobock will take reasonable steps to ensure the suggestions are correct, it is not obliged to provide technically accurate recommendations. Accordingly, Ottobock is not liable for possible technical errors in the recommendations except in the case of intent or gross negligence.

Your own technical responsibility for correct patient fittings remains unaffected by the non-binding recommendations.

1.4 To the extent that training requirements are specified for the use of the Ottobock software, the software may only be used by qualified personnel.

1.5 Third-party software is provided without warranty "as is". Ottobock does not provide any warranty of any kind (warranty of merchantability, warranty of fitness for a particular purpose or warranty of non-infringement of rights) with respect to any third-party software.

2. Licence

2.1 The Ottobock software is protected by national copyright laws in many countries and by international treaties. Ottobock will prosecute any violation of the copyrights it holds. You are only granted the right to use the Ottobock software to the extent required by law or expressly granted to you according to this licence agreement. Ottobock and/or its licensor(s) expressly reserve all ownership and/or other rights to the Ottobock software, including all copyrights, patents, business and trade secrets, trademarks and other intellectual property rights.

2.2 By accepting these Terms of Use, you are granted the non-exclusive and non-transferable right for 15 years to use the Ottobock software for your own purposes in accordance with its intended use, subject to any restrictions contained in these Terms of Use. "Own purposes" refers solely to the purposes of the respective contractual partner. In the case of medical supply companies or other companies that provide patient services related to Ottobock products (e.g. prosthesis adjustments), "own purposes" in terms of this licence agreement are also the purposes of the respective patient who wants to use the Ottobock products in accordance with their intended use.

2.3 You do not have the right to modify, edit, translate, rearrange, or otherwise alter the Ottobock Software nor to decompile, disassemble, or reverse engineer the Ottobock Software yourself or via third parties unless expressly permitted to do so by law.

2.4 You are authorised to install the Ottobock Software on several computers at the same time, or to use it on a network where the software can be accessed on more than one computer simultaneously. Making the software accessible to the public is not permitted. For the purposes of these Terms of Use, "computers" shall also be understood to mean those Ottobock products using the software according to its intended function.

3. Sublicences, assignment

Issuing sublicences for the use of the Ottobock Software is prohibited. Renting, leasing, loaning, or otherwise temporarily ceding the Ottobock software to a third party is also prohibited.

The permanent assignment of the usage rights granted to you is only possible when:

- the third party to whom the rights are to be assigned accepts the terms and conditions of this licence agreement,
- the entire Ottobock software, and not just parts thereof, is assigned, and
- you do not retain any copies of the Ottobock software, not even in the main memory or cache of your computer.

4. Liability

Ottobock is liable to you according to the provisions of the Product Liability Act; in case of intent or gross negligence; for the loss of life, physical injury or the impairment of health; where Ottobock issues any guarantees; and in other cases of mandatory legal liability – respectively pursuant to the applicable legal regulations. Damages shall be limited to an amount representing typically foreseeable damages. Damage compensation claims against Ottobock in case of slight negligence are excluded.

Any other claims for compensation by you against Ottobock – no matter on what legal grounds and especially due to material defects, defective title and/or the breach of other obligations arising from the contract on the part of Ottobock, its legal representatives, employees, or assistants or due to illegal acts – are excluded.

To the extent that the liability of Ottobock is limited or excluded by the preceding provisions, the same applies to the personal liability of the legal representatives, employees or vicarious agents of Ottobock.

The preceding provisions do not affect the burden of proof to your detriment. Claims for compensation on your part expire within the legal period of limitation, starting at the beginning of said period as established by law.

Ottobock is not liable for specific fitness or specific characteristics of the Ottobock software.

All claims shall be excluded if you fail to use and operate or modify the software expertly and properly and/or if you combine or operate the software with unsuitable components.

5. Applicable law and jurisdiction

This licence agreement shall be subject to the laws of the country in which the manufacturer is domiciled. The UN convention on contracts for the international sale of goods does not apply. The exclusive jurisdiction for all disputes arising from or in relation to this licence agreement is the registered office of the manufacturer.

6. Severability clause

Should one or more provisions of this agreement be or become ineffective or unenforceable in whole or in part, the validity of the remaining provisions of the agreement shall not be affected.

Any arrangement, change or addition (particularly commitments with respect to characteristics, features or the quality of the software product) in connection with these Terms of Use shall be deemed void unless made in writing and unless Ottobock's prior consent has been obtained.

This image shows a single sheet of white paper with horizontal ruling lines. The lines are evenly spaced and run across the width of the page. There are no margins, text, or other markings on the paper.



Otto Bock Healthcare Products GmbH
Brehmstraße 16 · 1110 Wien · Austria
T +43-1 523 37 86 · F +43-1 523 22 64
info.austria@ottobock.com · www.ottobock.com